



African Mineral Standards

MATRIX REFERENCE MATERIALS

Tel: +27 (0) 11 923 0800 Fax: +27 (0) 11 392 4715 web: www.amis.co.za
11 Gewel Street (off Hulley Road), D1 Isando Business Park, Kempton Park, 1609
P.O. Box 856, Isando, 1600, Gauteng, South Africa, a division of the Set Point Group

AMIS0430

Certified Reference Material

**Gold and Uranium Ore
Witwatersrand, South Africa**

Certificate of Analysis

**Recommended Concentrations and Limits^{1, 2}
(at two Standard Deviations)**

Certified Concentrations

Au Pb Collection	2.68	±	0.24	g/t
U M/ICP	113	±	8	ppm
S Comb/LECO	0.33	±	0.02	%
Specific Gravity	2.71	±	0.07	

1. Manufacturers recommended limits for use of the material as control samples, based on two standard deviations, calculated using "Between Laboratory" statistics for treatment of the data for trivial, non-trivial and technically invalid results. See sections 1, 10 and 13.
2. There is additional certified major element data presented on p2 and uncertified trace element data presented as an appendix.
3. Or, by applying a chemical conversion factor of $U \times 1.1793 = U3O8$; $U3O8$ by multi acid digestion: 133.26 ± 9.43 ppm



Directors: GJ Horsfield (CEO), MD Evers (CFO)(British), W Erasmus, Gerber, SJ Ingram
M McWha, N Robinson, V Singh, MH Snelling, J Vassiloudis

Major Element Recommended Concentrations and Limits (at two Standard Deviations)

Certified Concentrations

Al ₂ O ₃	2.80	±	0.03	%
CaO	0.19	±	0.01	%
Cr ₂ O ₃	0.12	±	0.01	%
Fe ₂ O ₃	2.03	±	0.05	%
K ₂ O	0.32	±	0.02	%
MnO	0.030	±	0.001	%
SiO ₂	92.3	±	0.9	%

Provisional Concentrations

MgO	0.11	±	0.03	%
TiO ₂	0.14	±	0.01	%
LOI	1.66	±	0.24	%

Informational Mean

Na ₂ O	0.06	±	0.05	%
-------------------	------	---	------	---

1. **Intended Use:** AMIS0430 can be used to check the analysis of gold and uranium ores, hosted by siliceous rocks, with a similar grade and matrix.

It is a matrix matched Certified Reference Material, fit for use as control samples in routine assay laboratory quality control when inserted within runs of samples and measured in parallel to the unknown. Its purpose is to monitor inter-laboratory or instrument bias and within lab precision. It can be used, indirectly, to establish the traceability of results to an SI system of units.

The recommended concentrations and limits for this material are property values based on a measurement campaign (round robin) and reflect consensus results from the laboratories that participated in the round robin.

Slight variations in analytical procedures between laboratories will reflect as slight biases to the recommended concentrations (see 19). Good laboratories will report results within the two standard deviation levels with a failure rate of <10 %.

The material can also be used for method development and for the calibration of equipment.

2. **Origin of Material:** This standard is a blend of Ventersdorp Contact Reef, Carbon Leader Reef and Vaal Reef material provided by Anglo Gold Ashanti in South Africa. It was made from a mixture of pulp reject sample material, collected during routine underground sampling, sourced from mine assay laboratories and blended down to a required grade with silica.

3. **Approximate Mineral and Chemical Composition:** The major gangue mineral is quartz with minor pyrite, uraninite and thucolite. Gold occurs primarily as discrete grains. Trace element chemistry data from 12 of the labs has been compiled but has not been certified. Summary statistics for this data are set out in the appendix.

4. Appearance: The material is a very fine powder. It is colored a Light Grey (Corstor 5Y 7/1).

5. Handling instructions: The material is packaged in Laboratory Packs and Explorer Packs that must be shaken or otherwise agitated before use. Normal safety precautions for handling fine particulate matter are suggested, such as the use of safety glasses, breathing protection, gloves and a laboratory coat.

6. Radioactivity: Shipments of this material require special labeling and placarding. AMIS0430 contains U (1.41Bq/g) and Th (0.063Bq/g) and is classified as EXEMPT MATERIAL in terms of "Safety Standards Series No. TS-R-1: Regulations for the Safe Transport of Radioactive Material, International Atomic Energy Agency, 2005, para 403, Table 1".

7. Method of Preparation: The material was crushed, dry-milled and air-classified to <54um. Wet sieve particle size analysis of random samples confirmed the material was 98.5% <54um. It was then blended in a bi-conical mixer, systematically divided and then sealed into 1kg Laboratory Packs. Explorer Packs are subdivided from the Laboratory packs as required. Samples were scientifically selected for homogeneity testing and third party analysis. Statistical analysis of both homogeneity and the consensus test results were carried out by independent statisticians.

8. Methods of Analysis requested:

1. Au – Pb collection ICP-OES or ICP-MS.
2. Multi-acid digest, including HF, ICP- OES or ICP-MS. Multi element scan to include U (M/ICP).
3. U XRF.
4. Majors (Al₂O₃, CaO, Cr₂O₃, Fe₂O₃, K₂O, MgO, MnO, Na₂O, SiO₂, TiO₂. LOI.) XRF fusion.
5. SG (gas pycnometer).
6. Additionally, XRF analyses were requested for the major elements and a multi-element multi acid digest and ICP scan was requested for the trace elements.

9. Information requested:

1. State aliquots used for all determinations.
2. Report all results for gold and uranium in ppm.
3. All results for major elements to be reported as oxides in percentages.
4. All results for multi-element scans to be reported in ppm.
5. Report all QC data, to include replicates, blanks and certified reference materials used.
6. State and provide brief description of analytical techniques used.

10. Method of Certification: Thirty laboratories were each given eight scientifically selected packages of sample. Twenty five of the laboratories submitted results in time for certification.

Final limits were calculated after first determining if all data was compatible within a spread normally expected for similar analytical methods done by reputable laboratories. Data from any one laboratory was then removed from further calculations when the mean of all analyses from that laboratory failed a "t test" of the global means of the other laboratories. The means and standard deviations were then re-calculated using all remaining data. Any analysis that fell outside of the new two standard deviations was removed from the ensuing data base. The mean and standard deviations were again calculated using the remaining data.

The “between-laboratory” standard deviation is used in the calculation to eliminate technically and statistically invalid data. Upper and lower limits are based on the standard deviation of the remaining data, which reflect individual analyses and can be used to monitor accuracy in routine laboratory quality control. This is different to limits based on standard deviations derived from grouped set of analyses (see 12), which provide important measures for precision and trueness, but which are less useful for routine QC.

Standards with an RSD of near or less than 5 % are termed “Certified”, RSD's of between near 5 % and 15 % are termed “Provisional”, and RSD's over 15 % are termed “Informational”.

11. Participating Laboratories: The 25 out of 30 laboratories that provided results timeously were (not in same order as in the table of assays):

1. ACME Analytical Laboratories Ltd CA
2. ALS Ammtec (Australia)
3. ALS Chemex Laboratory Group Johannesburg SA
4. ALS Chemex Laboratory Group Perth WA
5. ALS Chemex Laboratory Group Vancouver CA
6. Anglo Gold Ashanti - Navachab Gold Mine Laboratory Namibia
7. Anglo Gold Ashanti - Vaal River Laboratory SA
8. BV Rustenburg (South Africa)
9. Chromatech Services
10. Genalysis Laboratory Services (South Africa) Pty
11. Genalysis Laboratory Services (W Australia P)
12. Performance Laboratories Barberton
13. Performance Laboratories SA (Randfontein)
14. Performance Laboratories Zimbabwe
15. Rossing Uranium Limited
16. Set Point Laboratories (Isando) SA
17. SGS Australia Pty Ltd (Newburn) WA
18. SGS Geosol Laboratories Ltda (Brazil)
19. SGS Mineral Services Lakefield (Canada)
20. SGS Mwanza (Tanzania)
21. SGS Tarkwa (Ghana)
22. SGS Townsville (Australia)
23. SGS Vancouver (Canada)
24. Super Laboratory Services (Springs SA)
25. Ultra Trace (Pty) Ltd WA

12. Assay Data: Data as received from the laboratories for the important certified elements listed on p1 are set out below.

Lab Code	Au Pb Coll g/t	U M/ICP ppm	Al ₂ O ₃ XRF %	CaO XRF %	Cr ₂ O ₃ XRF %	Fe ₂ O ₃ XRF %	K ₂ O XRF %	LOI %	MgO XRF %	MnO XRF %	Na ₂ O XRF %	SiO ₂ XRF %	TiO ₂ XRF %	S Comb/LECO %	SG pyc
B	2.51	115	2.82	0.18	0.12	2.04	0.32	1.59	0.12	0.03	0.09	92.72	0.14	0.33	2.66
B	2.51	110	2.81	0.18	0.12	2.04	0.32	1.60	0.12	0.03	0.08	92.64	0.14	0.33	2.67
B	2.59	109	2.82	0.18	0.12	2.03	0.32	1.57	0.12	0.03	0.09	92.66	0.14	0.34	2.66
B	2.50	112	2.83	0.18	0.12	2.04	0.32	1.59	0.12	0.03	0.08	92.71	0.14	0.34	2.63
B	2.63	110	2.82	0.18	0.12	2.04	0.32	1.58	0.12	0.03	0.08	92.74	0.14	0.35	2.65
B	2.48	109	2.80	0.18	0.12	2.04	0.32	1.58	0.12	0.03	0.09	92.65	0.14	0.34	2.67
B	2.48	112	2.81	0.18	0.12	2.04	0.32	1.57	0.12	0.03	0.09	92.72	0.14	0.35	2.68
B	2.62	111	2.81	0.19	0.12	2.04	0.32	1.57	0.12	0.03	0.08	92.66	0.14	0.35	2.67
C	2.76	124	2.78	0.18	0.12	2.02	0.32	1.88	0.10	0.03	0.01	91.87	0.14		2.68
C	2.92	129	2.78	0.18	0.12	2.01	0.32	1.88	0.10	0.03	0.01	91.93	0.13		2.68
C	2.64	130	2.79	0.18	0.12	2.01	0.33	1.88	0.10	0.03	0.01	91.88	0.14		2.68
C	2.75	128	2.76	0.18	0.12	2.01	0.32	1.90	0.10	0.03	0.01	91.87	0.13		2.68
C	2.86	130	2.78	0.18	0.12	1.99	0.33	1.89	0.10	0.03	0.01	91.98	0.14		2.68
C	2.67	132	2.78	0.19	0.12	2.01	0.32	1.90	0.10	0.03	0.01	92.18	0.13		2.69
C	2.70	130	2.77	0.18	0.12	2.00	0.32	1.87	0.10	0.03	0.02	91.83	0.15		2.69
C	2.79	129	2.77	0.18	0.12	2.00	0.32	1.87	0.10	0.03		91.74	0.14		2.69

Assay data (cont)

Lab Code	Au Pb Coll g/t	U M/ICP ppm	Al ₂ O ₃ XRF %	CaO XRF %	Cr ₂ O ₃ XRF %	Fe ₂ O ₃ XRF %	K ₂ O XRF %	LOI %	MgO XRF %	MnO XRF %	Na ₂ O XRF %	SiO ₂ XRF %	TiO ₂ XRF %	S Comb/LECO %	SG pyc
D	2.56														
D	2.42														
D	2.41														
D	2.60														
D	2.62														
D	2.80														
D	2.83														
D	2.70														
E	2.56														
E	2.62														
E	2.61														
E	2.57														
E	2.56														
E	2.57														
E	2.58														
E	2.57														
G	2.47														
G	2.60														
G	2.41														
G	2.39														
G	2.37														
G	2.51														
G	2.42														
G	2.49														
I	2.80														
I	2.85														
I	2.93														
I	2.83														
I	2.85														
I	2.88														
I	2.67														
I	2.64														
J	2.93														
J	2.82														
J	2.81														
J	2.85														
J	2.85														
J	2.87														
J	2.86														
J	2.84														
K	2.57	107	2.85	0.19	0.11	2.05	0.32	1.64	0.12	0.03	0.04	92.70	0.14	0.33	
K	2.62	107	2.79	0.20	0.11	2.08	0.32	1.76	0.12	0.03	0.06	93.00	0.14	0.34	
K	2.71	107	2.79	0.19	0.11	2.07	0.33	1.77	0.14	0.03	0.04	93.80	0.14	0.33	
K	2.63	107	2.78	0.19	0.11	2.06	0.32	1.83	0.13	0.03	0.05	93.00	0.14	0.34	
K	2.79	105	2.87	0.19	0.11	2.06	0.33	1.98	0.12	0.04	0.04	92.70	0.13	0.33	
K	2.72	110	2.80	0.19	0.11	2.05	0.32	2.05	0.11	0.03	0.03	92.90	0.14	0.33	
K	2.57	110	2.80	0.19	0.11	2.06	0.32	1.84	0.13	0.03	0.03	92.80	0.14	0.33	
K	2.60	111	2.77	0.19	0.11	2.08	0.34	1.76	0.13	0.03	0.05	93.80	0.14	0.33	
L	2.71														
L	2.96														
L	2.63														
L	2.54														
L	2.57														
L	2.74														
L	2.56														
L	2.56														
N	2.44	120												0.38	2.73
N	2.69	122												0.42	2.73
N	2.53	123												0.38	2.74
N	2.75	119												0.38	2.72
N	2.84	120												0.39	2.74
N	2.71	121												0.37	2.73
N	2.52	120												0.37	2.72
N	2.72	120												0.38	2.73
O	2.57	108	2.79	0.19	0.11	2.01	0.32	1.49	0.11	0.03	0.09	91.60	0.13	0.33	2.72
O	2.84	110	2.77	0.18	0.11	2.02	0.32	1.57	0.11	0.03	0.09	91.70	0.13	0.33	2.71
O	2.73	112	2.76	0.19	0.11	2.01	0.32	1.66	0.11	0.03	0.09	91.80	0.13	0.32	2.70
O	2.72	112	2.79	0.19	0.11	2.03	0.32	1.55	0.11	0.03	0.10	91.90	0.13	0.34	2.71
O	2.81	104	2.78	0.19	0.11	2.02	0.31	1.72	0.11	0.03	0.09	91.80	0.13	0.34	2.70
O	2.75	108	2.78	0.19	0.11	2.02	0.32	1.47	0.11	0.03	0.09	91.90	0.13	0.33	2.71
O	2.93	112	2.79	0.19	0.12	2.02	0.32	1.56	0.11	0.03	0.09	91.90	0.13	0.33	2.70
O	2.45	112	2.79	0.19	0.11	2.02	0.32	1.73	0.12	0.03	0.09	91.80	0.13	0.33	2.72
Q	2.59														
Q	2.63														
Q	2.54														
Q	2.54														
Q	2.56														
Q	2.50														
Q	2.56														
Q	2.50														

Assay data (cont)

Lab Code	Au Pb Coll g/t	U M/ICP ppm	Al ₂ O ₃ XRF %	CaO XRF %	Cr ₂ O ₃ XRF %	Fe ₂ O ₃ XRF %	K ₂ O XRF %	LOI %	MgO XRF %	MnO XRF %	Na ₂ O XRF %	SiO ₂ XRF %	TiO ₂ XRF %	S Comb/LECO %	SG pyc
Q	2.59														
Q	2.63														
Q	2.54														
Q	2.54														
Q	2.56														
Q	2.50														
Q	2.56														
Q	2.50														
R	2.27	108													
R	2.74	111													
R	2.73	109													
R	2.62	112													
R	2.65	114													
R	2.70	113													
R	2.69	108													
R	2.62	111													
T	2.45														
T	2.48														
T	2.28														
T	2.44														
T	2.32														
T	2.47														
T	2.54														
T	2.52														
U	2.77	113													2.76
U	2.65	114													2.75
U	2.80	116													2.74
U	2.68	110													2.69
U	2.73	110													2.62
U	2.72	114													2.66
U	2.88	111													2.66
U	2.76	112													2.69
V	2.78	113	2.80	0.24	0.10	1.96	0.30	1.64	0.43	0.03	0.14	91.10	0.16		2.73
V	2.63	116	2.80	0.23	0.10	2.03	0.31	1.64	0.33	0.03	0.16	90.80	0.15		2.72
V	2.68	105	2.80	0.24	0.10	2.02	0.31	1.67	0.40	0.03	0.18	91.40	0.15		2.74
V	2.78	110	2.80	0.22	0.11	2.18	0.33	1.79	0.37	0.03	0.14	90.90	0.15		2.75
V	2.72	111	2.80	0.25	0.10	1.98	0.30	1.82	0.39	0.03	0.17	90.80	0.15		2.74
V	2.78	111	2.80	0.24	0.11	2.05	0.31	1.69	0.39	0.03	0.18	91.40	0.16		2.73
V	2.67	100	2.80	0.22	0.11	2.02	0.30	1.74	0.35	0.03	0.14	90.90	0.15		2.75
V	2.69	102	2.80	0.24	0.11	1.99	0.30	1.85	0.38	0.03	0.17	90.60	0.15		2.73
W	2.79	99	2.85	0.17	0.12	2.08	0.30	1.68		0.03		92.63	0.12	0.34	
W	2.64	101	2.82	0.18	0.12	2.03	0.31	1.62		0.03		92.46	0.13	0.34	
W	2.66	98	2.84	0.17	0.12	2.03	0.31	1.72		0.03		93.24	0.13	0.34	
W	2.63	99	2.82	0.17	0.12	2.03	0.30	1.65		0.03		92.58	0.12	0.34	
W	2.78	101	2.78	0.17	0.12	2.06	0.31	1.63		0.03		92.50	0.13	0.34	
W	2.64	101	2.81	0.18	0.12	2.07	0.32	1.66		0.03		93.38	0.13	0.33	
W	2.68	99	2.85	0.18	0.12	2.07	0.32	1.64		0.03		93.49	0.12	0.34	
W	2.78	95	2.85	0.17	0.12	2.03	0.31	1.73		0.03		92.12	0.12	0.34	
X	2.73	124													2.76
X	2.71	124													2.74
X	2.74	123													2.76
X	2.80	119													2.75
X	2.74	123													2.75
X	2.78	113													2.75
X	2.69	121													2.75
X	2.70	118													2.75
Y	2.24		2.80	0.19	0.12	2.01	0.32	1.52	0.10	0.03	0.08	92.60	0.13	0.32	
Y	2.50		2.82	0.19	0.12	2.03	0.32	1.52	0.10	0.03	0.07	92.70	0.14	0.33	
Y	2.15		2.80	0.19	0.12	2.01	0.32	1.48	0.11	0.03	0.08	92.70	0.13	0.33	
Y	2.33		2.80	0.19	0.12	2.00	0.32	1.53	0.11	0.03	0.08	92.70	0.14	0.33	
Y	2.43		2.79	0.19	0.12	2.01	0.32	1.51	0.10	0.03	0.08	92.70	0.13	0.33	
Y	2.50		2.79	0.19	0.12	2.01	0.32	1.51	0.10	0.03	0.09	92.70	0.14	0.33	
Y	2.59		2.79	0.19	0.11	2.01	0.32	1.49	0.10	0.03	0.08	92.80	0.13	0.33	
Y	3.13		2.81	0.19	0.12	2.02	0.32	1.52	0.10	0.03	0.08	92.70	0.13	0.33	
Z	2.44	85	2.71	0.18	0.12	2.02	0.31		0.12	0.03		92.07	0.13		
Z	2.43	85	2.72	0.19	0.12	2.02	0.31		0.13	0.03		92.05	0.13		
Z	2.42	86	2.70	0.19	0.12	2.02	0.31		0.12	0.03		91.95	0.13		
Z	2.45	85	2.74	0.18	0.13	2.02	0.30		0.13	0.04		91.99	0.14		
Z	2.46	85	2.75	0.18	0.12	2.03	0.30		0.14	0.04		91.98	0.14		
Z	2.45	86	2.79	0.19	0.12	2.01	0.30		0.14	0.04		91.67	0.13		
Z	2.37	85	2.73	0.19	0.12	2.01	0.30		0.14	0.03		92.07	0.14		
Z	2.46	85	2.76	0.19	0.13	2.02	0.30		0.15	0.03		91.87	0.14		
ZA	2.88	116	2.83	0.21	0.11	2.08	0.33	1.68	0.13	0.02	0.06	92.20	0.14	0.31	
ZA	2.76	115	2.84	0.20	0.12	2.07	0.33	1.61	0.13	0.02	0.04	92.50	0.13	0.32	
ZA	2.74	117	2.80	0.19	0.12	2.06	0.32	1.71	0.14	0.02	0.05	91.80	0.14	0.32	
ZA	2.80	116	2.80	0.19	0.12	2.09	0.32	1.66	0.13	0.02	0.05	92.40	0.14	0.31	
ZA	2.52	115	2.80	0.19	0.12	2.08	0.32	1.66	0.12		0.05	91.80	0.13	0.32	
ZA	2.65	116	2.82	0.19	0.12	2.08	0.33	1.67	0.11	0.02	0.05	92.30	0.13	0.32	
ZA	2.76	114	2.81	0.19	0.12	2.10	0.32	1.78	0.12	0.01	0.06	92.60	0.14	0.32	
ZA	2.75	116	2.78	0.19	0.12	2.06	0.33	1.63	0.14	0.02	0.05	91.60	0.13	0.32	

Assay data (cont)

Lab Code	Au Pb Coll g/t	U M/ICP ppm	Al ₂ O ₃ XRF %	CaO XRF %	Cr ₂ O ₃ XRF %	Fe ₂ O ₃ XRF %	K ₂ O XRF %	LOI %	MgO XRF %	MnO XRF %	Na ₂ O XRF %	SiO ₂ XRF %	TiO ₂ XRF %	S Comb/LECO %	SG pyc
ZB		109	2.76				0.35								
ZB		116	2.70				0.34								
ZB		115	2.76				0.35								
ZB		110	2.66				0.33								
ZB		106	2.78				0.35								
ZB			2.56				0.32								
ZB		106	2.63				0.33								
ZB		111	2.74				0.34								
ZC	2.73														
ZC	2.52														
ZC	2.40														
ZC	2.48														
ZC	2.69														
ZC	2.76														
ZC	2.68														
ZC	2.72														
ZD	2.54	113	2.81	0.18	0.12	2.04	0.32	1.58	0.09	0.03	0.08	92.50	0.13	0.35	2.65
ZD	2.59	112	2.81	0.18	0.11	2.06	0.32	1.58	0.09	0.03	0.08	92.52	0.13	0.34	2.71
ZD	2.41	114	2.80	0.18	0.12	2.03	0.32	1.57	0.09	0.03	0.07	92.29	0.13	0.35	2.64
ZD	2.39	115	2.80	0.18	0.12	2.03	0.32	1.56	0.09	0.03	0.08	92.30	0.13	0.35	2.70
ZD	2.78	115	2.81	0.18	0.12	2.04	0.32	1.55	0.10	0.03	0.08	92.53	0.13	0.35	2.78
ZD	2.38	115	2.80	0.18	0.12	2.04	0.32	1.56	0.09	0.03	0.08	92.41	0.13	0.34	2.72
ZD	2.41	114	2.81	0.18	0.12	2.03	0.32	1.56	0.09	0.03	0.08	92.54	0.13	0.35	2.74
ZD	2.51	113	2.80	0.18	0.12	2.03	0.32	1.55	0.09	0.03	0.08	92.51	0.13	0.35	2.72

13. Measurement of Uncertainty: (ref Dr Hugh Bartlett, Hugh Bartlett Consulting CC.)

The samples used in this certification process have been selected in such a way as to represent the entire batch of material and were taken from the final packaged units; therefore all possible sources of uncertainty (sample uncertainty and measurement uncertainty) are included in the final combined standard uncertainty determination.

The uncertainty measurement takes into consideration the between lab and the within lab variances and is calculated from the square roots of the variances of these components using the formula:

$$\text{Combined standard uncertainty} = \sqrt{(\text{between lab.var/no of labs}) + (\text{mean square within lab.var /no of assays})}$$

These uncertainty measurements may be used, by laboratories, as a component for calculating the total uncertainty for method validation according to the relevant ISO guidelines.

Analyte	Method	Unit	S ¹	σ _L ²	Sw ³	CSU ⁴
Au	Pb Coll	g/t	0.160	0.059	0.088	0.016
U	M/ICP	ppm	10.23	3.893	2.487	1.404
Al ₂ O ₃	XRF	%	0.045	0.014	0.010	0.005
CaO	XRF	%	0.017	0.005	0.004	0.002
Cr ₂ O ₃	XRF	%	0.006	0.004	0.002	0.002
Fe ₂ O ₃	XRF	%	0.031	0.023	0.011	0.009
K ₂ O	XRF	%	0.011	0.006	0.005	0.002
LOI		%	0.134	0.134	0.058	0.051
MgO	XRF	%	0.087	0.014	0.006	0.006
MnO	XRF	%	0.004	0.001	0.001	0.000
Na ₂ O	XRF	%	0.041	0.041	0.006	0.019
SiO ₂	XRF	%	0.644	0.469	0.190	0.179
TiO ₂	XRF	%	0.008	0.006	0.004	0.002
S	Comb/LECO	%	0.020	0.008	0.006	0.003
SG	pyc		0.037	0.031	0.017	0.012

1. S - Std Dev for use on control charts.
2. σ_L - Betw Lab Std Dev, for use to calculate a measure of accuracy.
3. Sw - Within Lab Std Dev, for use to calculate a measure of precision.
4. CSU - Combined Standard Uncertainty, a component for use to calculate the total uncertainty in method validation.

14. Certified values: The Certified, Provisional and Informational values listed on p1 of this certificate fulfill the AMIS statistical criteria regarding agreement for certification and have been independently validated by Margaret Fairhurst.

15. Metrological Traceability: The values quoted herein are based on the consensus values derived from statistical analysis of the data from an inter laboratory measurement program. Traceability to SI units is via the standards used by the individual laboratories the majority of which are accredited and who have maintained measurement traceability during the analytical process.

16. Certification: AMIS0430 is a new material.

17. Period of validity: The certified values are valid for this product, while still sealed in its original packaging, until notification to the contrary. The stability of the material will be subject to continuous testing for the duration of the inventory. Should product stability become an issue, all customers will be notified and notification to that effect will be placed on the www.amis.co.za website.

18. Minimum sample size: The majority of laboratories reporting used a 0.5g sample size for the ICP and a 30g sample size for the fire assay. These are the recommended minimum sample sizes for the use of this material.


19. Availability: This product is available in Laboratory Packs containing 1kg of material and Explorer Packs containing custom weights (from 50 to 250g) of material. The Laboratory Packs are sealed bottles delivered in sealed foil pouches. The Explorer Packs contain material in standard geochem envelopes, nitrogen flushed and vacuum sealed in foil pouches.

20. Recommended use: The data used to characterize this CRM has been scrutinized using outlier treatment techniques. This, together with the number of participating laboratories, should overcome any "inter-laboratory issues" and should lead to a very accurate measure for the given methods, notwithstanding the underlying assumption that what the good inter-laboratory labs reported was accurate. However an amount of bad data might have had an effect, resulting in limits which in some situations might be too broad for the effective monitoring of a single analytical method, laboratory or production process. Users should set their own limits based on their own data quality objectives and control measurements, after determining the performance characteristics of their own particular method, using a minimum of 20 analyses using this CRM. User set limits should normally be within the limits recommended on p1 and 2 of this certificate.

21. **Legal Notice:** This certificate and the reference material described in it have been prepared with due care and attention. However AMIS, Set Point Technology (Pty) Ltd, Mike McWha, and Margaret M. Fairhurst; accept no liability for any decisions or actions taken following the use of the reference material.


05 March 2015

Certifying Officers:



African Mineral Standards: _____

Michael McWha
BSc (Hons), FGSSA, FSAIMM, Pr.Sci.Nat

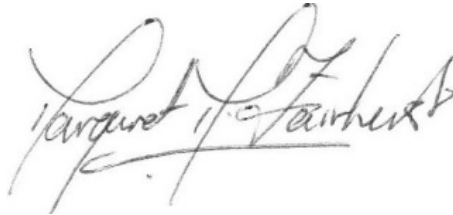

Geochemist: _____

Margaret M. Fairhurst, PG, MAusIMM
Oreval

Appendix – uncertified trace element statistics

Analyte	Method	Unit	Mean	2SD	RSD%	n
Ag	M/ICP	ppm	0.52	0.18	17.2	66
Al	M/ICP	%	1.5	0.13	4.4	86
As	M/ICP	ppm	70.7	7.8	5.5	86
Ba	M/ICP	ppm	77.5	6.4	4.1	91
Be	M/ICP	ppm	0.41	0.03	3.8	44
Bi	M/ICP	ppm	0.75	0.11	7.5	62
Ca	M/ICP	%	0.14	0.01	5.1	97
Cd	M/ICP	ppm	0.17	0.04	11.2	47
Ce	M/ICP	ppm	30.3	5.2	8.5	63
Co	M/ICP	ppm	16.6	1.6	4.9	76
Cr	M/ICP	ppm	596	346	29.0	96
Cs	M/ICP	ppm	0.74	0.16	10.8	56
Cu	M/ICP	ppm	206	19.7	4.8	101
Dy	M/ICP	ppm	2.1	0.09	2.2	8
Er	M/ICP	ppm	1.1	0.05	2.0	8
Eu	M/ICP	ppm	0.38	0.05	6.8	8
Fe	M/ICP	%	1.4	0.15	5.0	111
Ga	M/ICP	ppm	3.7	0.51	7.0	62
Ge	M/ICP	ppm	0.24	0.61	126.5	32
Hf	M/ICP	ppm	1.7	0.35	10.1	69
Ho	M/ICP	ppm	0.39	0.02	2.7	8
In	M/ICP	ppm	0.02	0.01	16.2	23
K	M/ICP	%	0.26	0.02	2.9	86
La	M/ICP	ppm	15.7	2.6	8.4	64
Li	M/ICP	ppm	7.5	1.2	7.8	76
Lu	M/ICP	ppm	0.13	0.02	7.4	31
Mg	M/ICP	%	0.06	0.01	8.8	89
Mn	M/ICP	ppm	253	14.7	2.9	78
Mo	M/ICP	ppm	3.2	0.31	4.8	75
Na	M/ICP	%	0.05	0.01	12.3	94
Nb	M/ICP	ppm	3.2	0.81	12.7	76
Nd	M/ICP	ppm	10.5	0.35	1.7	8
Ni	M/ICP	ppm	36.0	4.0	5.5	80
P	M/ICP	ppm	91.6	16.0	8.8	70
P ₂ O ₅	XRF	%	0.02	0.0	6.9	34
Pb	M/ICP	ppm	95.7	10.5	5.5	89
Pr	M/ICP	ppm	2.9	0.04	0.60	8
Rb	M/ICP	ppm	12.0	1.3	5.4	68
S	M/ICP	%	0.34	0.07	9.6	102
Sb	M/ICP	ppm	4.0	0.64	7.9	66
Sc	M/ICP	ppm	2.2	0.62	13.9	75
Si	M/ICP	%	43.2	0.33	0.4	8
Sm	M/ICP	ppm	2.2	0.13	3.0	8
Sn	M/ICP	ppm	2.0	0.26	6.7	69
Sr	M/ICP	ppm	23.2	2.3	4.9	82
Ta	M/ICP	ppm	1.4	0.41	15.2	68
Tb	M/ICP	ppm	0.34	0.03	3.9	29
Te	M/ICP	ppm	0.15	0.09	28.8	63
Th	M/ICP		15.5	2.3	7.3	75
Ti	M/ICP	%	0.07	0.02	13.5	90
Tl	M/ICP	ppm	0.14	0.04	13.3	50
U	XRF	ppm	110	4.7	2.2	45
U ₃ O ₈	XRF	ppm	132	5.6	2.1	24
V	M/ICP	ppm	23.9	2.0	4.1	87
W	M/ICP	ppm	1.1	0.18	8.5	54
Y	M/ICP	ppm	8.3	1.7	10.4	87
Yb	M/ICP	ppm	1.0	0.18	9.0	31
Zn	M/ICP	ppm	64.5	6.5	5.1	83
Zr	M/ICP	ppm	62.1	15.2	12.2	84